

CERTIFICATE OF ANALYSIS

19p19q/CON 19 Probe Set (Aqua/Red/Green; 20 Test Kit; 40 µl)

Catalog # 19P19Q-CHR19-20-ARG-R

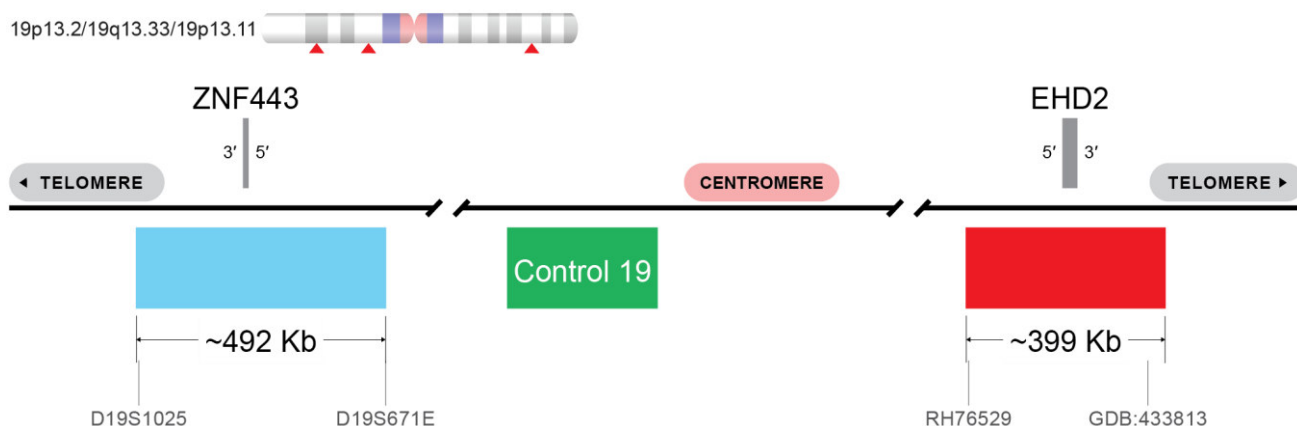


IMAGE NOT DRAWN TO SCALE

Fluorochrome	Localization
Aqua	19p13.2
Red	19q13.33
Green	19p13.11

Lot Number: 2025-05-21

Expiration Date: May 2027

Product Description – Quality Declaration

The **19p19q/CON 19 Probe Set** consists of DNA labeled in Spectrum Aqua, Spectrum Red and Spectrum Green. The DNA probe set hybridizes to chromosome 19p13.2 (Aqua), 19q13.33 (Red) and 19p13.11 (Green) in normal metaphase spreads and interphase nuclei.

Disclaimer

This probe set is for RESEARCH USE ONLY.

The probe set has NOT BEEN TESTED ON CLINICAL SAMPLES and is NOT VALIDATED.

Performance and analytical characteristics HAVE NOT been determined.

Chromosomal location based on GRCh37/hg19 build of human genome assembly.

Third party expiration studies were completed on concentrated probes only. We cannot guarantee the expiration date of probes mixed with buffer and stored reconstituted.