


CERTIFICATE OF ANALYSIS

CDK4/MDM2/Con 12 Probe Set (Orange/Green/Aqua; 20 Test Kit; 40 µl)

Catalog # CDK4-MDM2-CHR12-20-ORGRAQ

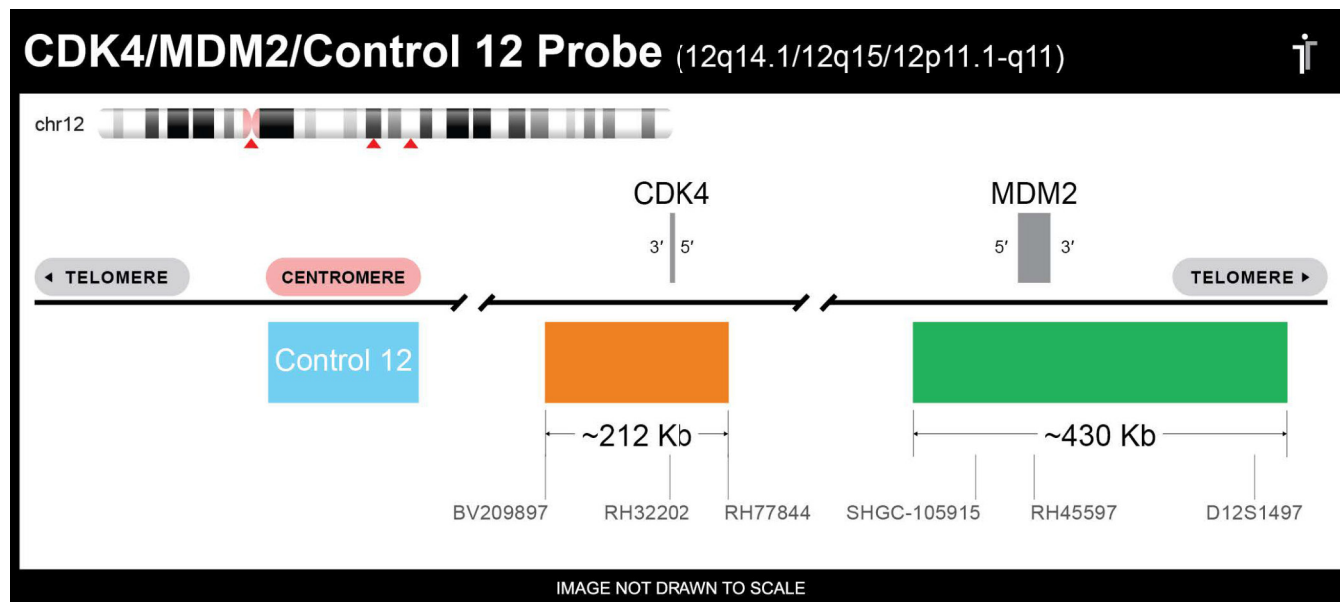

Fluorochrome	Localization
Orange	12q14.1
Green	12q15
Aqua	12p11.1-q11

Lot Number: 2022-08-10

Expiration Date: August 2025

Product Description – Quality Declaration

The **CDK4/MDM2/Con 12 Probe Set** consists of DNA labeled in Spectrum Orange, Spectrum Green and Spectrum Aqua. The DNA probe set hybridizes to chromosome 12q14.1 (Orange), 12q15 (Green) and 12p11.1-q11 (Aqua) in normal metaphase spreads and interphase nuclei.

Disclaimer

This probe set is for RESEARCH USE ONLY.

The probe set has NOT BEEN TESTED ON CLINICAL SAMPLES and is NOT VALIDATED.

Performance and analytical characteristics HAVE NOT been determined.

Chromosomal location based on GRCh37/hg19 build of human genome assembly.

Third party expiration studies were completed on concentrated probes only. We cannot guarantee the expiration date of probes mixed with buffer and stored reconstituted.