


CERTIFICATE OF ANALYSIS

CON 4/CON 10/CON 17 (RTU) Probe Set (Green/Red/Aqua; 10 Test Kit; 100 µl)

Catalog # CHR04-CHR10-CHR17-10-GRA-R-P

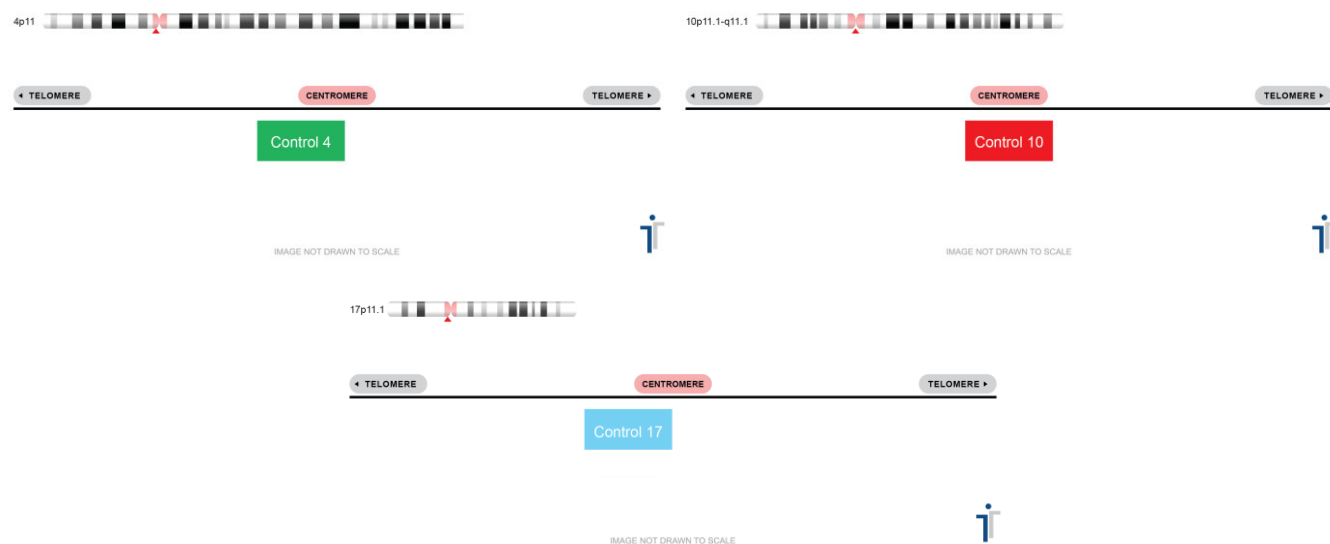

| Fluorochrome | Localization |
|--------------|---------------|
| Green | 4p11 |
| Red | 10p11.1-q11.1 |
| Aqua | 17p11.1 |

Lot Number: 2025-04-30

Expiration Date: May 2026

Product Description – Quality Declaration

The **CON 4/CON 10/CON 17 (RTU) Probe Set** consists of DNA labeled in Spectrum Green, Spectrum Red and Spectrum Aqua. The DNA probe set hybridizes to chromosome 4p11 (Green), 10p11.1-q11.1 (Red) and 17p11.1 (Aqua) in normal metaphase spreads and interphase nuclei.

Disclaimer

This probe set is for RESEARCH USE ONLY.

The probe set has NOT BEEN TESTED ON CLINICAL SAMPLES and is NOT VALIDATED.

Performance and analytical characteristics HAVE NOT been determined.

Chromosomal location based on GRCh37/hg19 build of human genome assembly.

Third party expiration studies were completed on concentrated probes only. We cannot guarantee the expiration date of probes mixed with buffer and stored reconstituted.