


# CERTIFICATE OF ANALYSIS

MECOM BA FISH Probe (Aqua/Green/Orange; 20 Test Kit; 40 µl)

Catalog # MECOMBA-20-AQGROR

## MECOM Break Apart Probe (3q26.2)

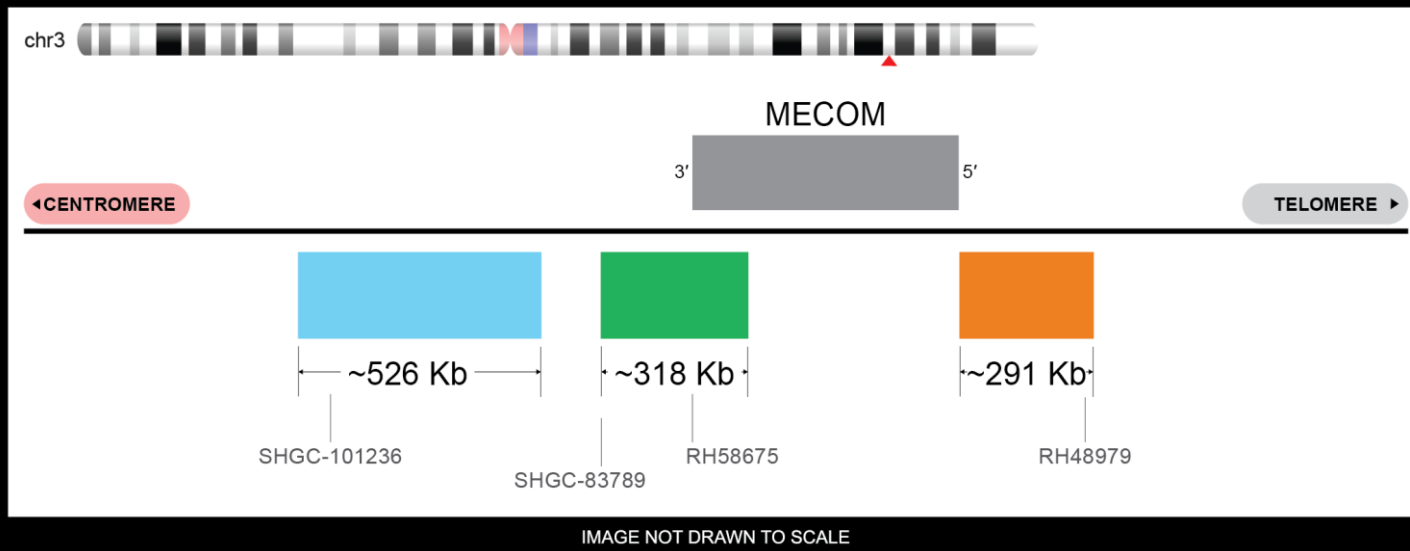

Fluorochrome	Localization
Aqua	3q26.2
Green	3q26.2
Orange	3q26.2

Lot Number: 2022-04-13

Expiration Date: 2025-03-24

### Product Description – Quality Declaration

The **MECOM BA FISH Probe** consists of DNA labeled in Spectrum Aqua, Spectrum Green, and Spectrum Orange. The DNA probe set hybridizes to chromosome 3q26.2 in normal metaphase spreads and interphase nuclei.

### Disclaimer

This probe set is CE MARKED in certain countries.

This probe set is for RESEARCH USE ONLY elsewhere.

The probe set has NOT BEEN TESTED ON CLINICAL SAMPLES and is NOT VALIDATED.

Performance and analytical characteristics HAVE NOT been determined.

Chromosomal location based on GRCh37/hg19 build of human genome assembly.

\*\*\*Third party expiration studies were completed on concentrated probes only. We cannot guarantee the expiration date of probes mixed with buffer and stored reconstituted.\*\*\*

EC REP MedNet EC-REP GmbH Borkstrasse 10 48163 Münster Germany