


CERTIFICATE OF ANALYSIS

MET Extended/Con 7 Probe Set (Red/Green; 20 Test Kit; 40 µl)

Catalog # MET-EXT-CHR07-20-REGR

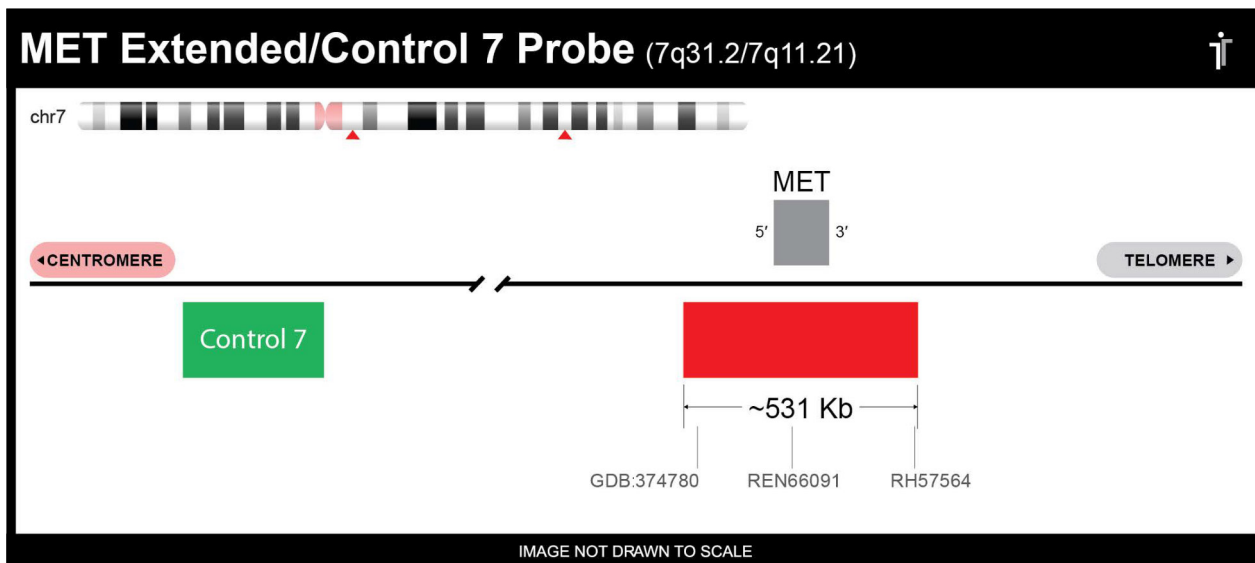

Fluorochrome	Localization
Red	7q31.2
Green	7q11.21

Lot Number: 2023-08-09

Expiration Date: August 2026

Product Description – Quality Declaration

The **MET Extended/Con 7 Probe Set** consists of DNA labeled in Spectrum Red and Spectrum Green. The DNA probe set hybridizes to chromosome 7q31.2 (Red) and 7q11.21 (Green) in normal metaphase spreads and interphase nuclei.

Disclaimer

This probe set is for RESEARCH USE ONLY.

The probe set has NOT BEEN TESTED ON CLINICAL SAMPLES and is NOT VALIDATED.

Performance and analytical characteristics HAVE NOT been determined.

Chromosomal location based on GRCh37/hg19 build of human genome assembly.

Third party expiration studies were completed on concentrated probes only. We cannot guarantee the expiration date of probes mixed with buffer and stored reconstituted.