

CERTIFICATE OF ANALYSIS

MYC BA/Control 8 Probe Set (Orange/Green/Aqua; 20 Test Kit; 40 µl)

Catalog # MYCBA-CHR08-20-ORGRAQ

MYC Break Apart/Control 8 Probe (8q24.21/8p11.1-q11.1)

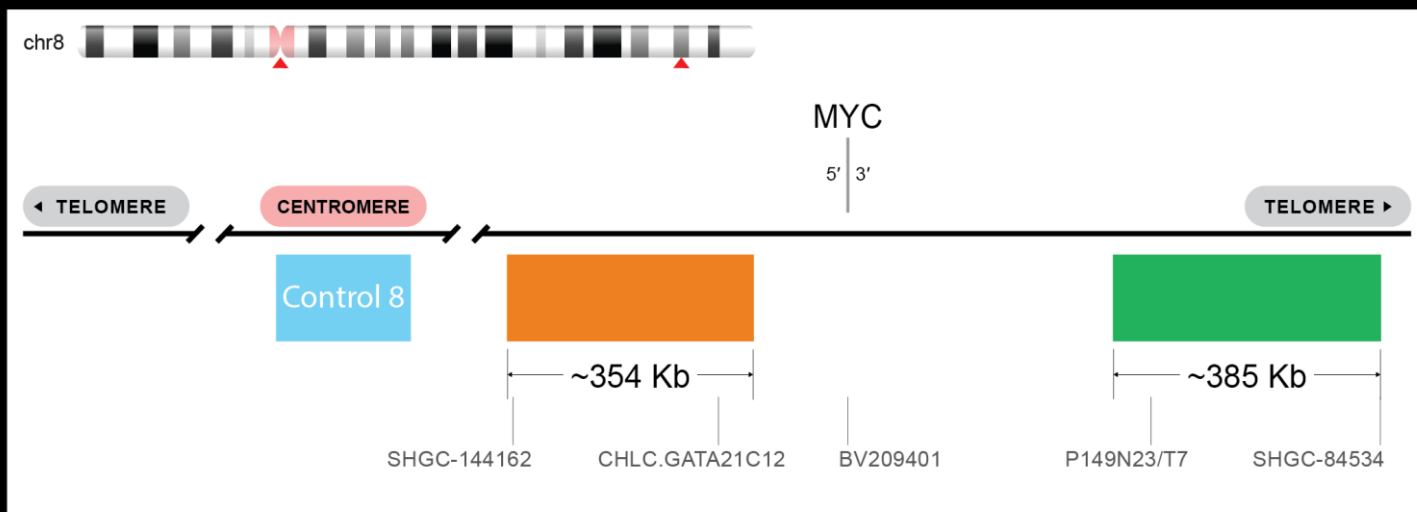


IMAGE NOT DRAWN TO SCALE

Fluorochrome	Localization
Orange	8q24.21
Green	8q24.21
Aqua	8p11.1-q11.1

Lot Number: 2023-04-26

Expiration Date: 2026-04-26

Product Description – Quality Declaration

The **MYC BA/Control 8 Probe Set** consists of DNA labeled in Spectrum Orange, Spectrum Green and Spectrum Aqua. The DNA probe set hybridizes to chromosome 8q24.21 (Orange and Green) and 8p11.1-q11.1 (Aqua) in normal metaphase spreads and interphase nuclei.

Disclaimer

This probe set is CE MARKED in certain countries.

This probe set is for RESEARCH USE ONLY elsewhere.

The probe set has NOT BEEN TESTED ON CLINICAL SAMPLES and is NOT VALIDATED.

Performance and analytical characteristics HAVE NOT been determined.

Chromosomal location based on GRCh37/hg19 build of human genome assembly.

Third party expiration studies were completed on concentrated probes only. We cannot guarantee the expiration date of probes mixed with buffer and stored reconstituted.



MedNet EC-REP GmbH Borkstrasse 10 48163 Münster Germany

