


CERTIFICATE OF ANALYSIS

MYCN/CON 2/ODC1 Probe Set (Red/Green/Aqua; 20 Test Kit; 40 µl)

Catalog # MYCN-CHR02-ODC1-20-RGA-R

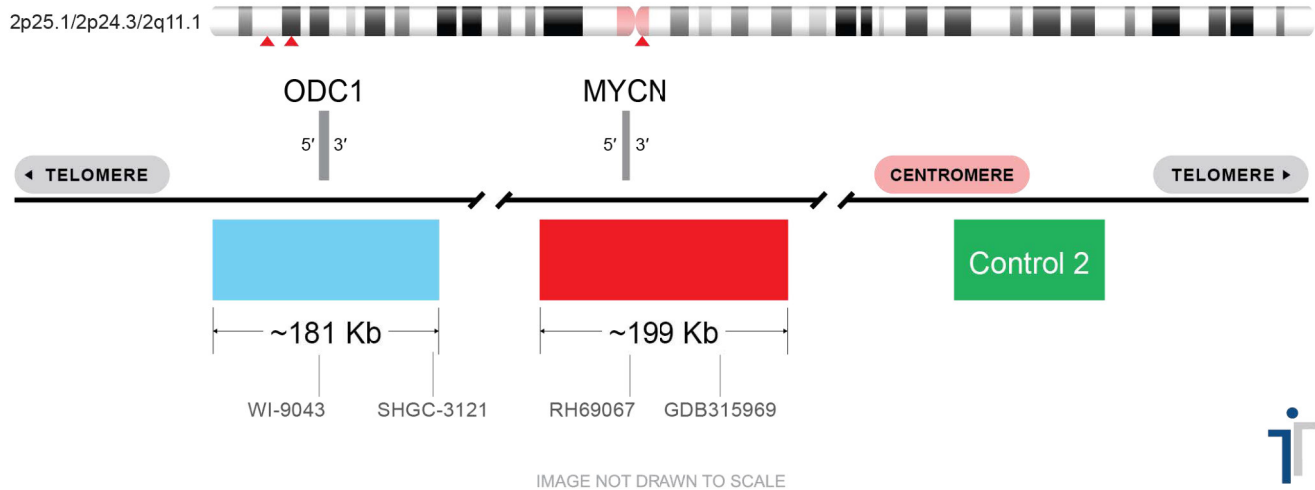

Fluorochrome	Localization
Red	2p24.3
Green	2q11.1
Aqua	2p25.1

Lot Number: 2025-02-12

Expiration Date: February 2027

Product Description – Quality Declaration

The **MYCN/CON 2/ODC1 Probe Set** consists of DNA labeled in Spectrum Red, Spectrum Green and Spectrum Aqua. The DNA probe set hybridizes to chromosome 2p24.3 (Red), 2q11.1 (Green) and 2p25.1 (Aqua) in normal metaphase spreads and interphase nuclei.

Disclaimer

This probe set is for RESEARCH USE ONLY.

The probe set has NOT BEEN TESTED ON CLINICAL SAMPLES and is NOT VALIDATED.

Performance and analytical characteristics HAVE NOT been determined.

Chromosomal location based on GRCh37/hg19 build of human genome assembly.

Third party expiration studies were completed on concentrated probes only. We cannot guarantee the expiration date of probes mixed with buffer and stored reconstituted.