


# CERTIFICATE OF ANALYSIS

**TFCP2 BA Probe Set (Green/Orange; 10 Test Kit; 20 µl)**

**Catalog # TFCP2BA-10-GROR**

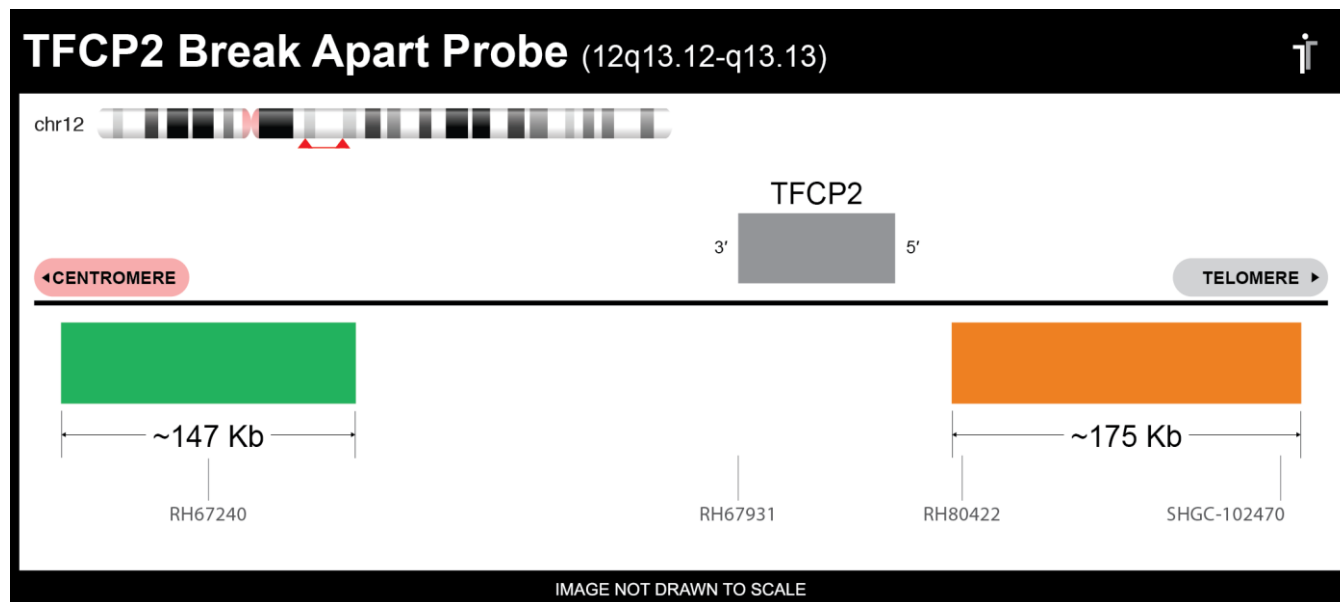

Fluorochrome	Localization
Green	12q13.12
Orange	12q13.13

**Lot Number:** 2021-11-10

**Expiration Date:** November 2024

## Product Description – Quality Declaration

The **TFCP2 BA Probe Set** consists of DNA labeled in Spectrum Green and Spectrum Orange. The DNA probe set hybridizes to chromosome 12q13.12-q13.13 in normal metaphase spreads and interphase nuclei.

## Disclaimer

This probe set is for RESEARCH USE ONLY.

The probe set has NOT BEEN TESTED ON CLINICAL SAMPLES and is NOT VALIDATED.

Performance and analytical characteristics HAVE NOT been determined.

Chromosomal location based on GRCh37/hg19 build of human genome assembly.

\*\*\*Third party expiration studies were completed on concentrated probes only. We cannot guarantee the expiration date of probes mixed with buffer and stored reconstituted.\*\*\*