


CERTIFICATE OF ANALYSIS

ZNF217/Con 20 Probe Set (Red/Green; 50 Test Kit; 100 µl)

Catalog # ZNF217-CHR20-50-REGR

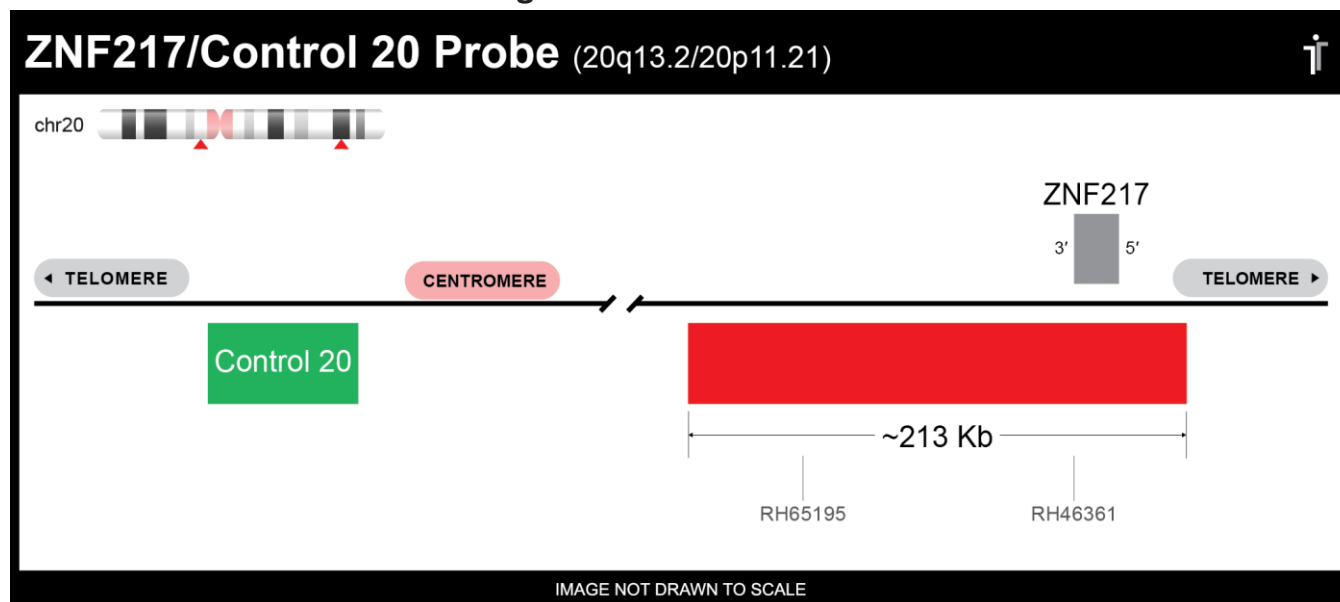

Fluorochrome	Localization
Red	20q13.2
Green	20p11.21

Lot Number: 2021-11-03

Expiration Date: November 2024

Product Description – Quality Declaration

The **ZNF217/Con 20 Probe Set** consists of DNA labeled in Spectrum Red and Spectrum Green. The DNA probe set hybridizes to chromosome 20q13.2 (Red) and 20p11.21 (Green) in normal metaphase spreads and interphase nuclei.

Disclaimer

This probe set is for RESEARCH USE ONLY.

The probe set has NOT BEEN TESTED ON CLINICAL SAMPLES and is NOT VALIDATED.

Performance and analytical characteristics HAVE NOT been determined.

Chromosomal location based on GRCh37/hg19 build of human genome assembly.

Third party expiration studies were completed on concentrated probes only. We cannot guarantee the expiration date of probes mixed with buffer and stored reconstituted.